(A)

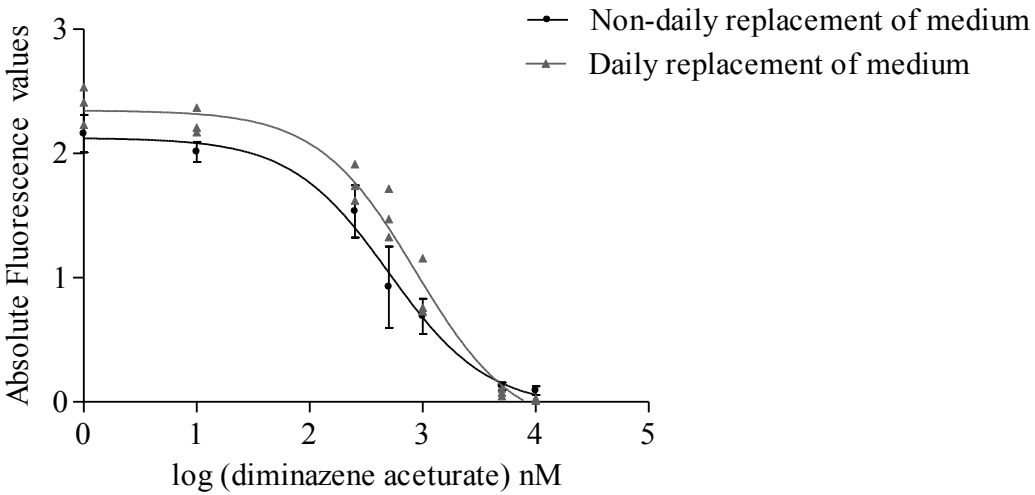
Non-daily replacement of medium
Daily replacement of medium
Absolute Fluorescence values
log (diminazene aceturate) nM
0
1
2
3
4
5

(B)

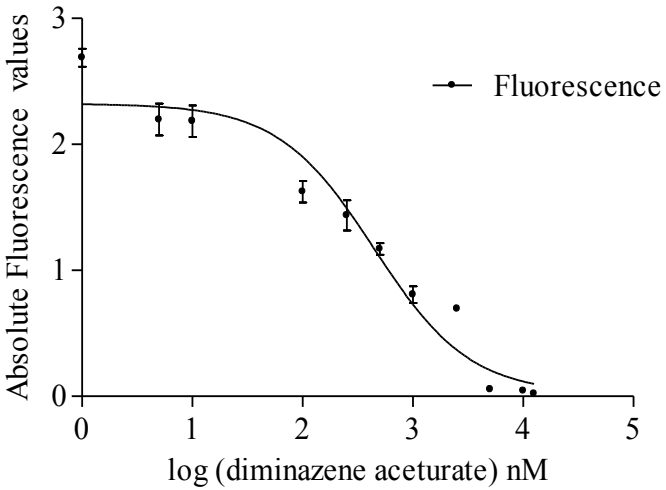
Fluorescence
Absolute Fluorescence values
log (diminazene aceturate) nM
0
1
2
3
4
5

(C)

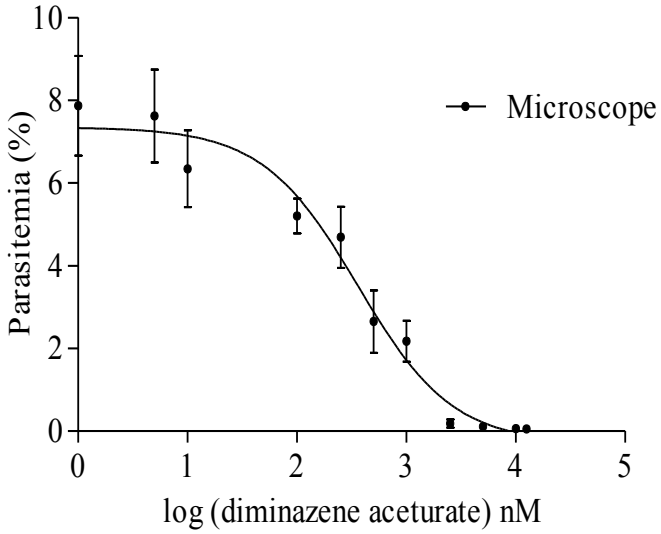
Microscope
Parasitemia (%)
log (diminazene aceturate) nM
0
2
4
6
8
10
1
3
5

S4_Fig.